

Figure 1. Perspective drawing of the ultrasound transducer interface

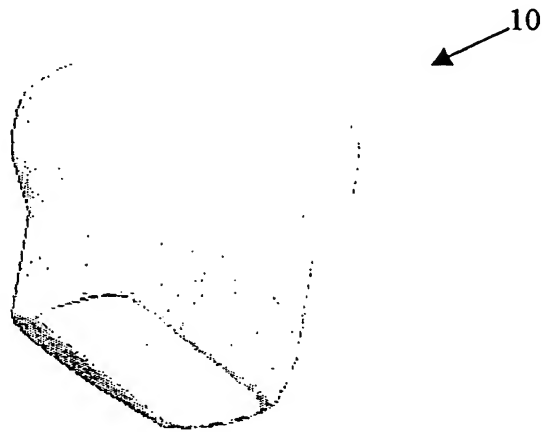


Figure 2. Cross-section drawing of interface device

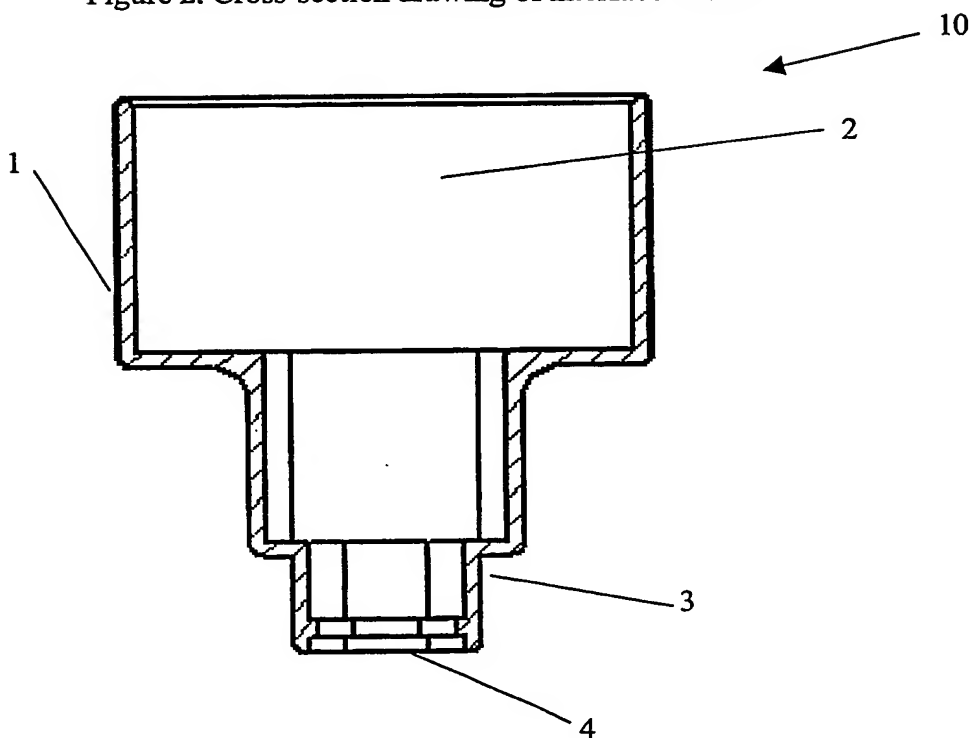


Figure 3. Cross-Sectional view of device with molded window component.

